


Kentech Instruments Ltd.

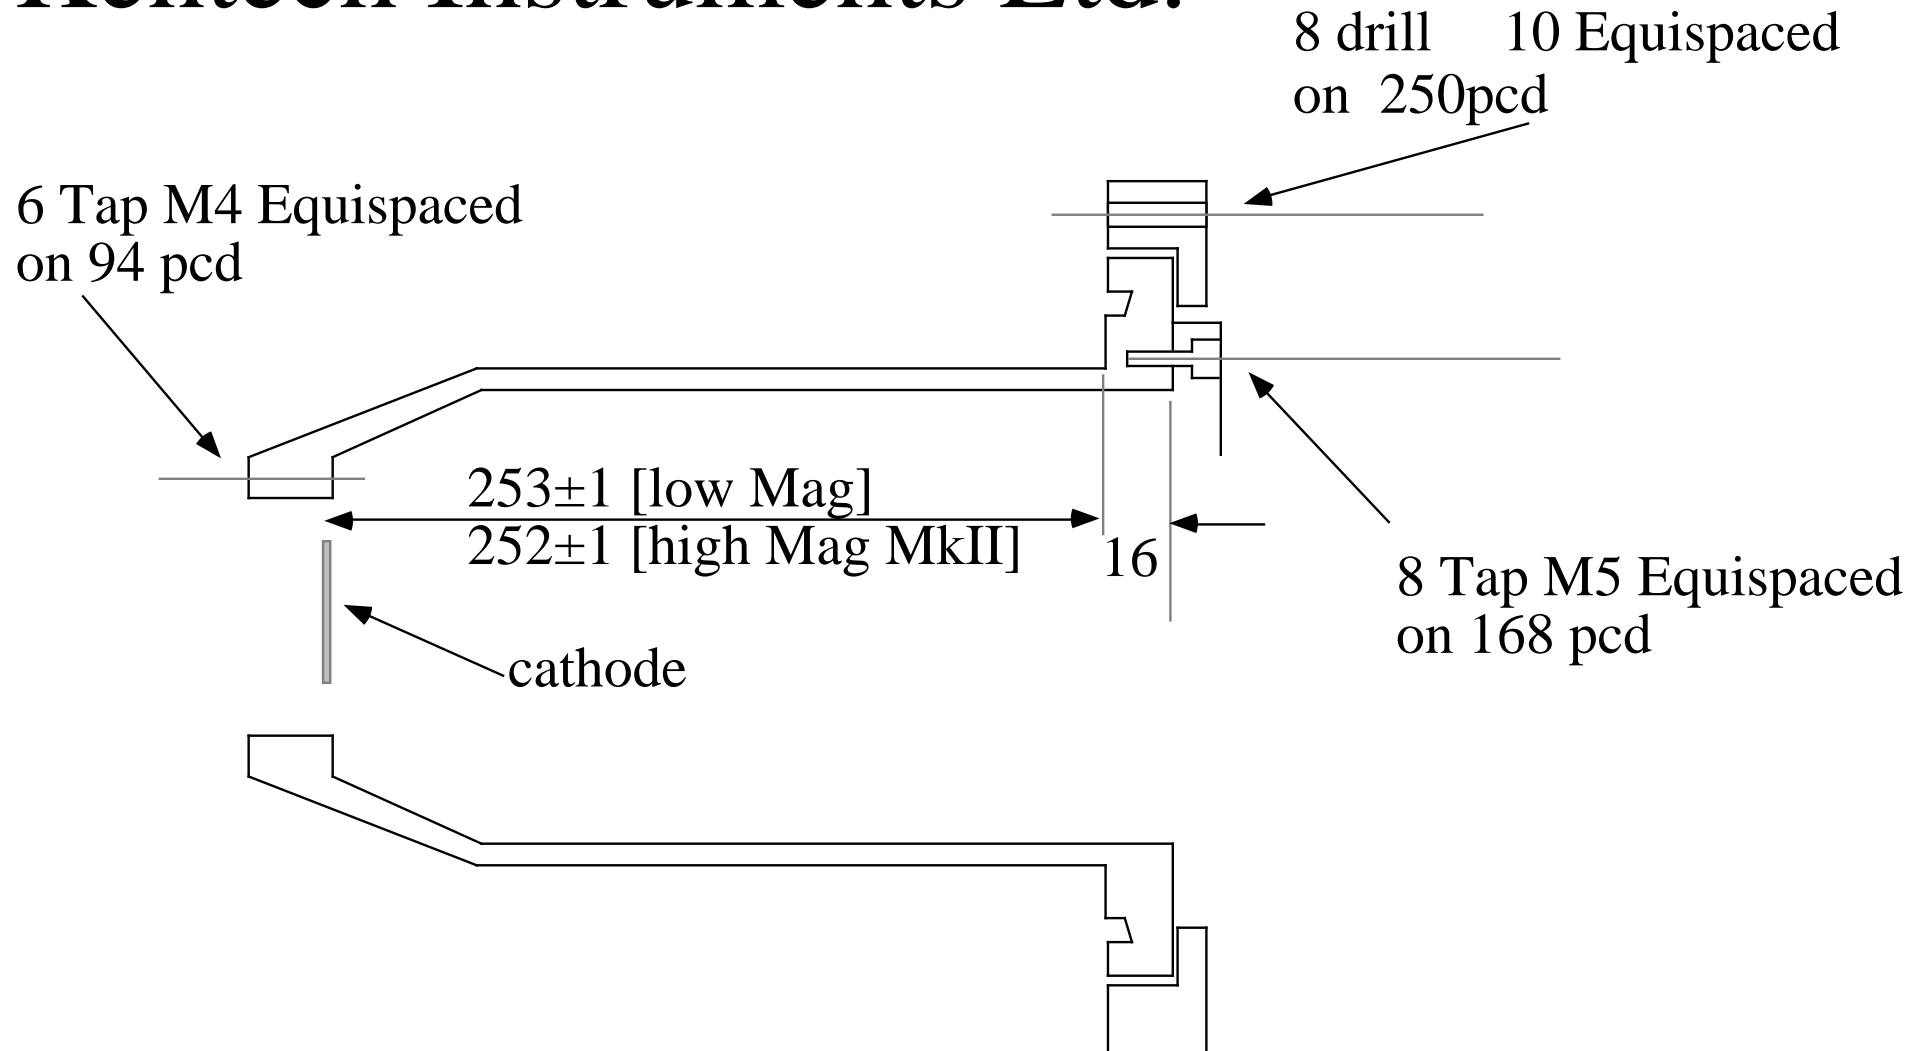

Dimensions in mm.

Exact position of cathode depends upon cathode to mesh spacer in use. The position of the extraction mesh is fixed.

For reflection cathodes the cathode to mesh gap can be up to 1cm or so.

Figures given are for standard spacers.